

“PEEK” – ING into the Future! A Literature Review on Use of PEEK polymer in Prosthodontics

Neda Essa M. Al Omar¹, Khalil Ibrahim A. Idris², Halah Athman A. Alaqi², Ahmed Yahya A. Juraybi³, Saurabh Jain^{4*}

¹General Dentist (The Ministry of Health), Jazan, KSA

²General Dentist (Private Clinic), Jazan, KSA

³General Dentist (The Ministry of Health), Albaha, KSA

⁴Assistant Professor, Department of Prosthetic Dental Science, College of Dentistry, Jazan University, Jazan, KSA

DOI: [10.36348/sjodr.2021.v06i01.006](https://doi.org/10.36348/sjodr.2021.v06i01.006)

| Received: 24.12.2020 | Accepted: 04.01.2021 | Published: 09.01.2021

*Corresponding author: Saurabh Jain

Abstract

Advances in material science and technologies has helped dentist in proving the best possible treatment options to the patients. Due to its superior Physical and mechanical properties, Polyetheretherketone (PEEK) has been tried in various aspects of dentistry. The use of PEEK in prosthodontics ranges from crowns, removable partial dentures, fixed partial denture and maxillofacial prosthesis and implant superstructures. The aim of this study is to review and evaluate the use of PEEK polymer in the field of Prosthodontics. The indexed English literature published was systematically searched for studies on PEEK and its use in prosthodontics. Full text of all the articles were studied to select final articles for this review. Suitable mechanical properties and biocompatibility is making PEEK a favorable material for use in prosthodontics. Further long-term In vivo studies are required, for this material to replace other conventional materials, used in prosthodontics.

Keywords: PEEK, Polyetheretherketone, Metal-free RPD, CAD/CAM prostheses.

Copyright © 2021 The Author(s): This is an open-access article distributed under the terms of the Creative Commons Attribution **4.0 International License (CC BY-NC 4.0)** which permits unrestricted use, distribution, and reproduction in any medium for non-commercial use provided the original author and source are credited.

INTRODUCTION

Advances in material science and technologies has helped dentist in proving the best possible treatment options to the patients. For any new dental material to be used successfully in advanced dentistry, it should fulfill the basic minimal requirements. These requirements include biocompatibility, plaque repulsion, esthetic acceptability, and physical properties similar to natural oral and dental structures. Polyetheretherketone (PEEK) (-C₆H₄-OC₆H₄-O-C₆H₄-CO-)n is a semi crystalline polycyclic aromatic polymer which was developed in late ninety's. PEEK was used as a substitute for metal implants for vertebral surgery [1-3]. Later with advancement in material science, carbon fiber reinforced PEEK material was used prosthetic material in artificial hip joints [4]. PEEK is under trial in various aspects of clinical dentistry. Due to its unique physical and mechanical properties, PEEK is a promising material for dental applications especially in prosthodontics. The use of

PEEK in prosthodontics ranges from crowns, removable partial dentures, fixed partial denture and maxillofacial prosthesis and implant superstructures [5-9]. The aim of this study is to review and evaluate the use of PEEK polymer in the field of Prosthodontics.

MATERIALS AND METHODS

The indexed English literature published up to 30th November 2020, was systematically searched for studies on PEEK and its use in prosthodontics. Databases searched were PubMed, the Cochrane Library, and MEDLINE (OVID). Two reviewers independently screened and shortlisted the relevant studies based on predefined inclusion and exclusion criteria detailed in Table 1. Key terms were used while searching articles. Reference lists of relevant articles were manually searched to search more relevant articles. Full text of all the articles were studied to select final articles for this review.

Table-1: Inclusion and Exclusion Criteria

Inclusion criteria	Exclusion criteria
Literature in English language	Animal studies
Human clinical studies	Literature in language other than English
In vitro studies	Articles not related to use of peek in Prosthodontics
Comparison between PEEK and different materials	Letters to the editor
	Unpublished abstracts, reports, commentaries, Company literatures

RESULTS

398 articles were collected after initial search. Number of articles left after removing duplicates were 181. After reviewing titles and abstracts 37 articles were eligible for this study (Figure-1). These articles were read in details and relevant information was documented.

Table-2 describes the Division of studies on use of PEEK in dentistry. Out of total 93 studies, 37 (39.8%) are on use of PEEK in prosthodontics, 29 (31.2%) are on use of PEEK in implant dentistry, 10 (10.8%) are on use of PEEK in other dental specialties, while 17 (18.3%) studies discuss Physical and mechanical properties of PEEK.

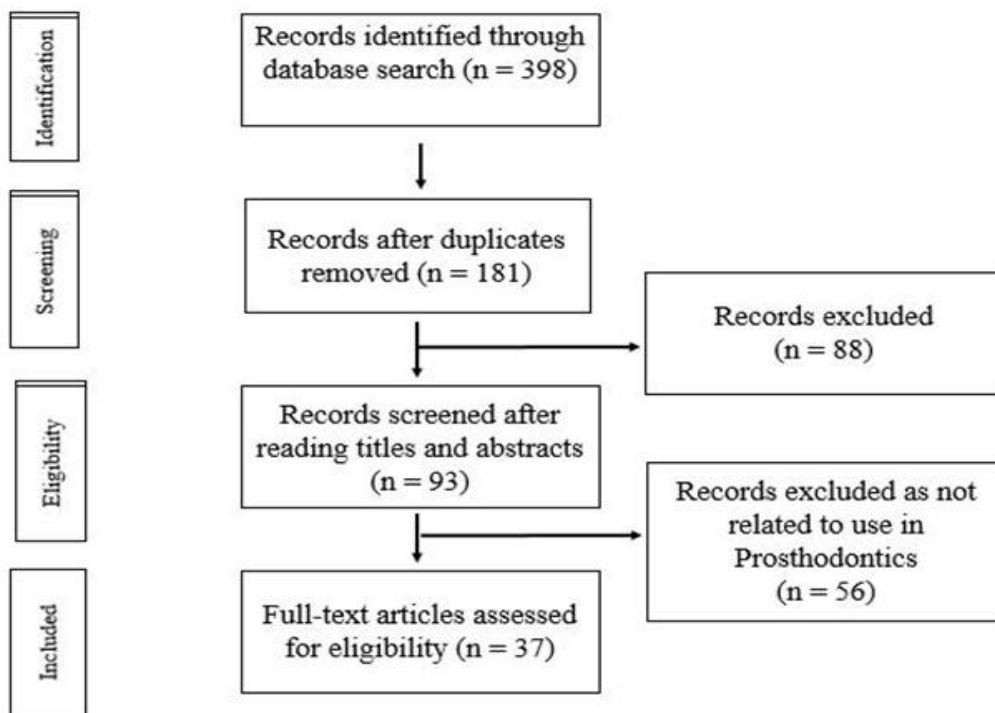


Fig-1: Article Selection Strategy

Table-2: Division of studies on use of PEEK in dentistry

S. No	Division of studies on use of PEEK in dentistry	Total Number of articles (N=93)
A)	Use of PEEK in Prosthodontics	37 (39.8%)
	(i) Removable Partial Dentures (RPD)	7 (18.9%)
	(ii) Fixed Partial Dentures (FPD)	6 (16.2%)
	(iii) Crowns	20 (54.1%)
	(iv) Maxillofacial Prosthesis	4 (10.8%)
B)	PEEK in implant dentistry	29 (31.2%)
C)	Physical and mechanical properties of PEEK	17 (18.3%)
D)	PEEK in other dental Specialties	10 (10.8%)

DISCUSSION

PEEK Polymer as RPD Framework

Due to superior mechanical properties, PEEK is commonly used for fabricating removable partial denture (RPD) framework. Computer aided designing

and computer aided manufacturing (CAD-CAM) can be used for this accurate fabrication of RPD frameworks [5]. Various studies reported that PEEK containing fillers (20% ceramic fillers) (BioHPP) have improved physical properties and can be used successfully for

fabricating RPD frameworks [6, 10, 11]. PEEK is lighter in weight, more aesthetic and causes less torquing forces on abutment tooth. Zoidis P *et al.*, [12] & Tannous F *et al.*, [13] reported that the RPD direct retainers made of PEEK have a lower retentive force compared to those made from Co–Cr.

PEEK as crown and FPD

PEEK reinforced with other inorganic fillers is used for fabricating both provisional and definitive crowns and fixed partial dentures (FPDs) [7, 14]. Studies reported high fracture resistance [15], high patient comfort and acceptability and better marginal fit [16, 17] of CAD/CAM provisional crowns and FPDs made up of PEEK. Studies by Stawarczyk B *et al.*, [18] and Skirbutis G *et al.*, [19], reported that due to its grayish color, PEEK is not suitable for monolithic aesthetic restorations of anterior teeth. Veneering by composite should be done to achieve better esthetic results.

PEEK as Obturator

PEEK polymer has some of the properties which are highly desirable for any material to be used for fabricating Obturator prosthesis. One of the most important properties is weight. Many techniques are documented in the literature to make Obturator prosthesis (made from Poly methyl Methacrylate) lighter in weight [20]. Whereas, prosthesis made from PEEK are very light as compared to other material [21].

Weightlessness along with biocompatibility and ease of polishing will make PEEK polymer as material of choice in near future.

PEEK as intraradicular post-core material

PEEK has been tried as intraradicular post-core material. Lee *et al.*, in their study found that post made from PEEK have high fracture resistance as compared to other commonly used post and core materials and there are less chances of root fracture when using PEEK [8].

PEEK as superstructure for implants

Studies by Adler *et al.*, showed that Fatigue strength for BioHPP is very high and can be used as super structure for implants [9]. Thus PEEK can be used as superstructure for implants retained prosthesis.

PEEK as dental implant material

There is no common consensus in the literature with respect to osseointegrating properties of unmodified PEEK, when compared to conventional implant materials such as zirconia and titanium. Few studies suggest that there is no significant difference [22], while others suggest that osseointegration is poorer than conventional implant materials [23, 24]. Various methods (Surface treatment, Coating and Bio composite) are suggested in the literature to improve the osseointegration of PEEK polymer [25].

Table-3: Use of PEEK in Prosthodontics: Advantages, Disadvantages and Limitations

Use of PEEK in Prosthodontics	Advantages	Disadvantages	Limitations
As RPD framework Peek containing fillers (20% ceramic fillers) (BioHPP)	<ul style="list-style-type: none"> Lighter weight Aesthetic Less torquing forces on abutment tooth 	PEEK direct retainers have lower retentive force compared to Co–Cr retainers	Paucity of long-term In vivo studies
As crown and FPD PEEK reinforced with other inorganic fillers	<ul style="list-style-type: none"> High fracture resistance High patient comfort and acceptability Better marginal fit of provisional crowns 	Grayish brown color. Should be layered with composite to achieve aesthetic results.	Paucity of long-term In vivo studies
As Obturator	<ul style="list-style-type: none"> Lighter weight Biocompatibility Ease of polishing 	-	Paucity of long-term In vivo studies
As intraradicular post-core material	<ul style="list-style-type: none"> High fracture resistance Less chances of root fracture 	-	Paucity of long-term In vivo studies
As superstructure for implants BioHPP appears to be appropriate for implant superstructures	<ul style="list-style-type: none"> High Fatigue strength (1200N) 	-	Paucity of long-term In vivo studies
As dental implant material	No common consensus in the literature with respect to osseointegrating properties of PEEK when compared to conventional implant materials such as zirconia and titanium.		Paucity of long-term In vivo studies

CONCLUSION

The current article reviews the use of PEEK in prosthodontics. Suitable mechanical properties and biocompatibility is making PEEK a favorable material for use in prosthodontics. Further long-term In vivo studies are required, for this material to replace other conventional materials, used in prosthodontics.

REFERENCES

- Toth, J. M., Wang, M., Estes, B. T., Scifert, J. L., Seim, H. B., 3rd, & Turner, A. S. (2006). Polyetheretherketone as a biomaterial for spinal applications. *Biomaterials*, 27(3), 324–334. <https://doi.org/10.1016/j.biomaterials.2005.07.011>
- Kurtz, S. M., & Devine, J. N. (2007). PEEK biomaterials in trauma, orthopedic, and spinal implants. *Biomaterials*, 28(32), 4845–4869. <https://doi.org/10.1016/j.biomaterials.2007.07.013>
- Pokorný, D., Fulín, P., Slouf, M., Jahoda, D., Landor, I., & Sosna, A. (2010). Polyetheretherketone (PEEK)--II. část: Poznatky o využití v klinické praxi [Polyetheretherketone (PEEK). Part II: application in clinical practice]. *Acta chirurgiae orthopaedicae et traumatologiae Cechoslovaca*, 77(6), 470–478.
- Ma, R., & Tang, T. (2014). Current strategies to improve the bioactivity of PEEK. *International journal of molecular sciences*, 15(4), 5426–5445. <https://doi.org/10.3390/ijms15045426>
- Harb, I. E., Abdel-Khalek, E. A., & Hegazy, S. A. (2019). CAD/CAM Constructed Poly (etheretherketone) (PEEK) Framework of Kennedy Class I Removable Partial Denture: A Clinical Report. *Journal of prosthodontics: official journal of the American College of Prosthodontists*, 28(2), e595–e598. <https://doi.org/10.1111/jopr.12968>
- Seferis, J. C. (1986). Polyetheretherketone (PEEK): Processing-structure and properties studies for a matrix in high performance composites. *Polymer Composites*, 7(3), 158–169.
- Zhou, L., Qian, Y., Zhu, Y., Liu, H., Gan, K., & Guo, J. (2014). The effect of different surface treatments on the bond strength of PEEK composite materials. *Dental materials: official publication of the Academy of Dental Materials*, 30(8), e209–e215. <https://doi.org/10.1016/j.dental.2014.03.011>
- Lee, K. S., Shin, J. H., Kim, J. E., Kim, J. H., Lee, W. C., Shin, S. W., & Lee, J. Y. (2017). Corrigendum to "Biomechanical Evaluation of a Tooth Restored with High Performance Polymer PEKK Post-Core System: A 3D Finite Element Analysis". *BioMed research international*, 2017, 7196847. <https://doi.org/10.1155/2017/7196847>
- Bathala, L., Majeti, V., Rachuri, N., Singh, N., Gedela, S. (2019). The Role of Polyether Ether Ketone (Peek) in Dentistry - A Review. *Journal of Medicine and Life*, 12(1):5-9.
- Katzer, A., Marquardt, H., Westendorf, J., Wening, J. V., & von Foerster, G. (2002). Polyetheretherketone--cytotoxicity and mutagenicity in vitro. *Biomaterials*, 23(8), 1749–1759. [https://doi.org/10.1016/s0142-9612\(01\)00300-3](https://doi.org/10.1016/s0142-9612(01)00300-3)
- Rivard, C. H., Rhalmi, S., & Coillard, C. (2002). In vivo biocompatibility testing of peek polymer for a spinal implant system: a study in rabbits. *Journal of biomedical materials research*, 62(4), 488–498. <https://doi.org/10.1002/jbm.10159>
- Zoidis, P., Papataniasiou, I., & Polyzois, G. (2016). The Use of a Modified Poly-Ether-Ether-Ketone (PEEK) as an Alternative Framework Material for Removable Dental Prostheses. A Clinical Report. *Journal of prosthodontics: official journal of the American College of Prosthodontists*, 25(7), 580–584. <https://doi.org/10.1111/jopr.12325>
- Tannous, F., Steiner, M., Shahin, R., & Kern, M. (2012). Retentive forces and fatigue resistance of thermoplastic resin clasps. *Dental materials: official publication of the Academy of Dental Materials*, 28(3), 273–278. <https://doi.org/10.1016/j.dental.2011.10.016>
- Schmidlin, P. R., Stawarczyk, B., Wieland, M., Attin, T., Hämmerle, C. H., & Fischer, J. (2010). Effect of different surface pre-treatments and luting materials on shear bond strength to PEEK. *Dental materials : official publication of the Academy of Dental Materials*, 26(6), 553–559. <https://doi.org/10.1016/j.dental.2010.02.003>
- Stawarczyk, B., Eichberger, M., Uhrenbacher, J., Wimmer, T., Edelhoff, D., & Schmidlin, P. R. (2015). Three-unit reinforced polyetheretherketone composite FDPs: influence of fabrication method on load-bearing capacity and failure types. *Dental materials journal*, 34(1), 7–12. <https://doi.org/10.4012/dmj.2013-345>
- Abdullah, A. O., Tsitrou, E. A., & Pollington, S. (2016). Comparative in vitro evaluation of CAD/CAM vs conventional provisional crowns. *Journal of applied oral science : revista FOB*, 24(3), 258–263. <https://doi.org/10.1590/1678-775720150451>
- Sinha, N., Gupta, N., Reddy, K. M., & Shastry, Y. M. (2017). Versatility of PEEK as a fixed partial denture framework. *Journal of Indian Prosthodontic Society*, 17(1), 80–83. <https://doi.org/10.4103/0972-4052.197941>
- Stawarczyk, B., Beuer, F., Wimmer, T., Jahn, D., Sener, B., Roos, M., & Schmidlin, P. R. (2013). Polyetheretherketone-a suitable material for fixed dental prostheses?. *Journal of biomedical materials research. Part B, Applied biomaterials*, 101(7), 1209–1216. <https://doi.org/10.1002/jbm.b.32932>
- Skirbutis, G., Dzingutė, A., Masiliūnaitė, V., Šulcaitė, G., & Žilinskas, J. (2017). A review of

- PEEK polymer's properties and its use in prosthodontics. *Stomatologija*, 19(1), 19–23.
20. Jain, S., Aggarwal, A., Shetty, S. (2014). An innovative technique for fabrication of a hollow maxillary resection prosthesis: A Case Report. *Indian J Dent Sci*, 6(5), 55-57.
 21. Costa-Palau, S., Torrents-Nicolas, J., Brufau-de Barberà, M., & Cabratosa-Termes, J. (2014). Use of polyetheretherketone in the fabrication of a maxillary obturator prosthesis: a clinical report. *The Journal of prosthetic dentistry*, 112(3), 680–682.
<https://doi.org/10.1016/j.prosdent.2013.10.026>
 22. Sagomyants, K. B., Jarman-Smith, M. L., Devine, J. N., Aronow, M. S., & Gronowicz, G. A. (2008). The in vitro response of human osteoblasts to polyetheretherketone (PEEK) substrates compared to commercially pure titanium. *Biomaterials*, 29(11), 1563–1572.
<https://doi.org/10.1016/j.biomaterials.2007.12.001>
 23. Najeeb, S., Bds, Z. K., Bds, S. Z., & Bds, M. S. (2016). Bioactivity and Osseointegration of PEEK Are Inferior to Those of Titanium: A Systematic Review. *The Journal of oral implantology*, 42(6), 512–516. <https://doi.org/10.1563/aaid-joi-D-16-00072>
 24. Olivares-Navarrete, R., Gittens, R. A., Schneider, J. M., Hyzy, S. L., Haithcock, D. A., Ullrich, P. F., Schwartz, Z., & Boyan, B. D. (2012). Osteoblasts exhibit a more differentiated phenotype and increased bone morphogenetic protein production on titanium alloy substrates than on poly-ether-ether-ketone. *The spine journal: official journal of the North American Spine Society*, 12(3), 265–272.
<https://doi.org/10.1016/j.spinee.2012.02.002>
 25. AlOtaibi, N., Naudi, K., Conway, D., & Ayoub, A. (2020). The current state of PEEK implant osseointegration and future perspectives: a systematic review. *European cells & materials*, 40, 1–20.
<https://doi.org/10.22203/eCM.v040a01>.